

INSTRUCTION AND MAINTENANCE MANUAL

AUTOMATIC SERVICING EQUIPMENT FOR AIR CONDITIONING SYSTEMS

MODEL: 328 ICEGARD BLU





1 CONTENTS

		ON	
		N OF THE UNIT	
4.1		ed useed	
4.2		cation of the unit and its components	
4.3		cal characteristics	
4.3	3.1 Main c	characteristics	9
4.3	3.2 Power	r and consumption	9
4.3	3.3 Noise I	levels	9
4.3	3.4 Techni	nical data concerning the instruments used	9
5	SAFETY	-	10
5.1	General	ıl safety rules	10
5.	1.1 Specio	al instructions for units to be used with R-1234yf	11
5.2	Guidelir	nes for handling refrigerants	
5.2		ary of terms	
5.2	2.2 Precai	iutions for refrigerant storage	13
5.2		ition of the refrigerant and the system	
5.2		cling capacity	
5.2	· - / -	ral considerations	
5.3		devices	
5.4		g environment	
		9 311 1 311 1 311	
6.1		king and checking the components	_
6.2		ndling and storage	
6.3		ation for use	
6.4	•)	
6.5	•	ng Off	
6.6		I tank filling phase	
6.7		g of incondensable gases	
	_	g of incondensable gases	
, 7.1		ction/error messages	
7.2		n messages	
		DESCRIPTION	
8.1		ing Modalities	
8.2	•	ly of programming	
8.3	•		
	•		
7 9.1		nition developed services	
7.1 9.2	•	atic Program	
7.2 9.2		el Search (Data base)	
		,	
9.2 9.3		nodels	
		ogram	
9.4	•	mming injection oil-UV phase	
9.4		natic Oil - UV injection	
9.4		al Oil - UV injection	
9.4		d Oil – Uv injection	
		OGRAMMED CYCLES	
10.1		ery/recycling phase	
10.2		n phase	
10.3	Oil – UV	/ injection	39



10.3.1	Automatic Oil – UV injection	39
10.3.2	Timed Oil – UV injection	39
10.3.3	Manual Oil – UV injection	40
10.4	Charging phase	41
11 OTH	ER MENUS	42
11.1	Filling internal tanks	42
11.2	Diagnosis	
11.2.1	Hoses empting	
11.2.2	Suction of refrigerant through the A/C System	
11.3	PRINTER	
11.3.1	Repeat service report	
11.3.2	Personalization of service report heading	46
11.4	Service	
11.4.1	Setting language	
11.4.2	Date and hour	
11.4.3		
11.5	A4 Printout	
11.6	Back up/restore	
11.7	Exporting service history	
11.8	Exporting refrigerant IN/OUT	
	ITIONAL FUNCTIONS	
12.1	Leak test with nitrogen (N2)	
12.2	Flushing	
12.3	kit POE "Hybrid"	
12.3.1	kit POE "Hybrid" enabling	
12.3.2	1	
	P FOR LONG PERIODS	
	NTENANCE	
14.1	Changing the vacuum pump oil	
14.2	Filter replacement	
	OSAL	
15.1	Environmental disposals	
15.2	Disposal of recycled material	
16 FLO	N DIAGRAM	60



2 INTRODUCTION

Congratulations on your choice! The unit you have purchased is a direct result of our experience in this sector and it will guarantee you long-term, efficient operation.

This unit has been designed and built to ensure long lasting, high-level operating reliability with maximum safety for operators. ISC Systems has carefully selected all materials and components (combined with the adoption of generous safety margins) together with a management procedure based on continuous controls which, from the introduction of the product into the company, through storage and use in the workshop, will ensure the absence of damage, deterioration or malfunctions.

A further guarantee is provided by the strict factory tests and inspections to which the unit is subjected.

The user is therefore only responsible for ensuring proper use of the unit in accordance with the instructions found in this manual

It is essential that this unit is used according to the intended use specified in this manual. ISC Systems cannot be held responsible for any damage to persons, animals and/or objects due to improper use, different to that illustrated in this instruction manual.

ISC Systems reserves the right to modify the technical characteristics and appearance of the product without prior notification.

This unit is designed for use in commercial environments and light industry.

The purpose of this manual is to supply the user with all the information needed to use the unit, from the time of purchase through to the disposal of the said unit.

This manual may contain printing errors.

The manual has been devised to ensure maximum support for the personnel assigned to use and the maintenance of the unit. However, for any special needs or requests for technical assistance or spare parts, please contact our Customer Service department.

Customer Assistance Service

ISC Systems.
Via Comunità Carnica, 9
33029 Villa Santina (UD)
Tel. +39-0433-748425
info@iscsystems.it



3 GUARANTEE

ISC Systems assures the highest quality both of the row materials and the technical procedures used in the production of its Equipment.

- Check the integrity of the whole package at the receipt of the goods. Claims for transport damage must be notified to the Forwarder Company within 8 days from the date of good's receipt.
- 2. The Product ISC Systems is under warranty if it has been used and kept on the basis of what already specified in the user manual offered with the Unit.
- 3. Interventions under warranty on ISC Systems Products are performed by official ISC Systems Distributors or specialized personnel authorized by ISC Systems; transport charges are at Customer's charge.
- 4. For any contact with ISC Systems Distributors or with ISC Systems directly, it is always necessary to mention the Model and the Serial Number of the Equipment which are reported in the identification card.
- 5. The Product is granted by ISC Systems against possible defects of the materials employed for their construction starting from 12 months production date: components which will be considered defective will be replaced free of charge. Further extensions of the warranty terms offered by the ISC Systems Distributor will be granted exclusively under his responsibility.
- 6. Replacement of components during the warranty period of time, does not extend the validity of the same warranty but only of the detective component that will be covered by 3 months.
- 7. We suggest You to preserve the original package.
- 8. The operation of calibration of the pressure sensor as well as for load cells, the replacement of quick connectors or external plastic panels, electro valves cleaning and replacement of gaskets for HP /LP filling hoses must be considered as a procedure of installation or ordinary maintenance.

Warranty is not provided in such following cases:

- Components subjected to ordinary wear and tear of the equipment like for example: power cable and sockets, external plastic panels, stickers, external HP/LP charge hoses, HP/LP quick connectors and all components usually subjected to ordinary wear and tear.
- Damages caused by negligence, improper maintenance, transport, storage, uncorrect use.
- Anomalies on functioning caused by the use of the same Unit on A/C Equipment previously treated with "A/C Leak substances", fluids for flushing or which contain lubricants or refrigerants not suitable to the specific use or use of universal dye different from the type suggested by ISC Systems



4 DESCRIPTION OF THE UNIT

4.1 Intended use

ICEGARD BLU is an automatic unit designed solely for use in automobile air-conditioning system maintenance.


Recovery, recycling, vacuum, oil injection, UV injection, system filling, flushing and leak test with nitrogen are the functions that *ICEGARD BLU* is capable of carrying out in complete safety and providing top-level performance in its category.



The unit is not designed to handle disposal operations! (see Chap. 4.2.1 Glossary of terms)

4.2 Identification of the unit and its components


The **ICEGARD BLU** is composed of a series of internal and external components as shown in the following photographs.

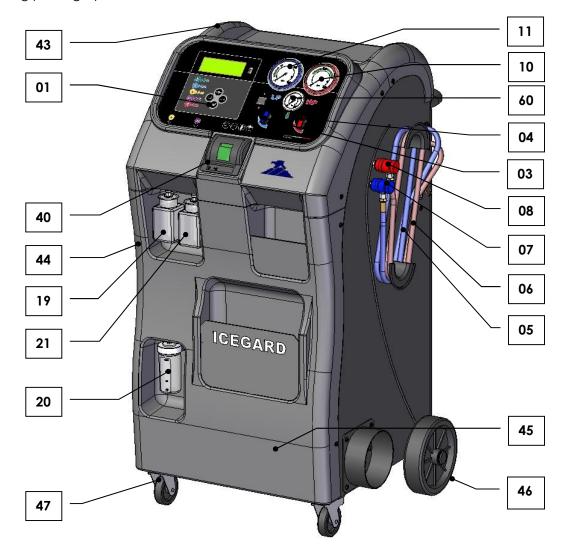



ITEM	DESCRIPTION
1	LOGIC BOARD
2	USB PORT
3	LOW PRESSURE VALVE
4	HIGH PRESSURE VALVE
5	BLUE FLEXIBLE HOSE 3000
	RED FLEXIBLE HOSE 3000 (5000 HD)
7	LP QUICK CONNECTOR (5000 HD)
8	HP QUICK CONNECTOR
9	FLUSHING VALVE
10	D80 HP GAUGE
11	D80 LP GAUGE
12	PRESSURE SENSOR –1/20 BAR
13	KPL DISTILLER
14	OIL SEPARATOR
15	FILTER
16	COMPRESSOR
17	VACUUM PUMP
	FLUSHING HP COUPLING
25	RUBBER HOSE
26	RUBBER HOSE
27	FAN CONDENSER
28	HP SAFETY PRESSURE SWITCH
29	MECHANICAL FILTER
30	NITROGEN VALVE
31	M/F CHECK VALVE
32	CHECK VALVE
33	INCONDENSABLES DISCHARGE VALVE
34	INTERNAL CONTAINER
35	UNCONDENSABLE DISCARGE RING
40	PRINTER
42	DOUBLE POLE SWITCH
43	UPPER PANEL
44	CONTROL PANEL
45	LOWER PANEL
46	REAR WHEEL
47	REVOLVING WHEEL WITH BRAKE
48	FILTER/COMPRESSOR VALVE
	-
18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 40 42 43 44 45 46 47	60 Kg LOAD CELL OIL INJECTION CONTAINER OIL DRAIN CONTAINER UV INJECTION CONTAINER EXPANSION VALVE NITROGEN LP COUPLING FLUSHING HP COUPLING RUBBER HOSE RUBBER HOSE FAN CONDENSER HP SAFETY PRESSURE SWITCH MECHANICAL FILTER NITROGEN VALVE M/F CHECK VALVE CHECK VALVE INCONDENSABLES DISCHARGE VALVE INTERNAL CONTAINER UNCONDENSABLE DISCARGE RING PRINTER DOUBLE POLE SWITCH UPPER PANEL CONTROL PANEL LOWER PANEL REAR WHEEL REVOLVING WHEEL WITH BRAKE



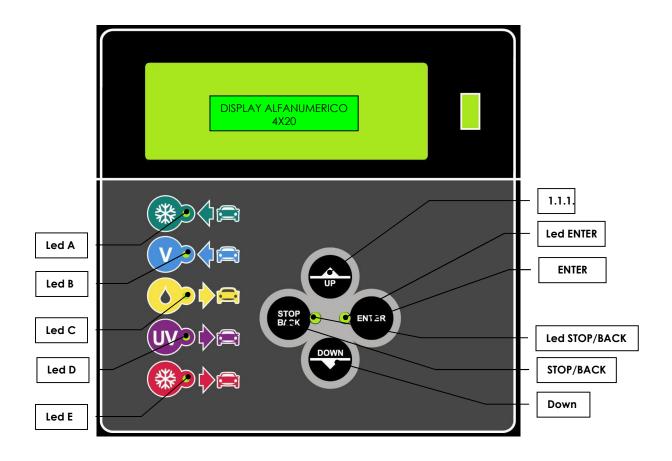

2	
DOWN	Input of programming parameters, descending order /
	visualization pressure sensor
UP	Input of programming parameters, ascending order /
	visualization counters
ENTER	Confirm function or menu
STOP/BACK	Select function or menu (Escape o Back)
Led S	Power ON pilot light
Led STOP/BACK	Function change pilot light
Led A	Recycling phase indicator
Led B	Vacuum phase indicator
Led C	Oil injection phase indicator
Led D	UV injection phase indicator
Led E	Filling phase indicator



4.3 Technical characteristics

4.3.1 Main characteristics

Refrigerant: R134a or R1234yf

verify on identification plate

Electronic refrigerant scales: Precision +/- 10 g

Electronic vacuum gauge: ≤ 2 %

LP and HP gauges: KI. 1.6

ICEGARD BLU internal container capacity: 12,4 L

ICEGARD BLU HD internal container capacity: 40 L

Maximum refrigerant storable quantity: 10 Kg

Maximum refrigerant storable quantity HD version: 38 Kg
Compressor cubic capacity: 9cc
Compressor cubic capacity for HD version: 14cc

Vacuum pump flow rate:

4.2 m³/h 2.5 CFM - 70 l/min

Vacuum pump flow rate HD version:

13 m3/h - 3.5 CFM - 226 l/min

Filtering station: 2 filters combined
Dimensions: 1200x697x562 mm

Weight: 95 Kg
Weight HD version: 105 Kg

4.3.2 Power and consumption

Supply voltage: 230 V 50/60 Hz

Power: **770 W**

4.3.3 Noise levels

The unit's noise levels have been measured from the operator's position (front).

Measurements recorded: 53.5 dB (A)

Distance of microphone from the ground:

1.40 m

Distance of microphone from the unit:

1.00 m

4.3.4 Technical data concerning the instruments used

(conforming to IEC 651 group 1 requirements).

B & K precision integrating noise meter.

Pre-polarised condenser microphone.

Acoustic level gauge.



5 SAFETY

The advanced technology adopted on design and production of *ICEGARD BLU* makes this unit extremely simple and reliable performing of all operations.

The user is therefore not exposed to any risk provided that the general safety rules indicated below are followed and that the unit is properly used and maintained.


5.1 General safety rules

- This unit is intended for use by **professionally trained operators** only. Such operators must have a knowledge of refrigeration, refrigeration systems, refrigerants and the potential hazards that units under high pressure may cause.
- To ensure safe and proper use of the unit, the User must read this manual carefully.
- Check that the type of refrigerant in the A/C system is the same expected for the unit.
- Use only the type of refrigerant expected for the unit, see the identification plate located near the main switch of the unit. Mixing with other types of refrigerant will seriously damage the cooling and refrigeration systems, as well as the service unit.
- It is required that suitable protective equipment such as goggles and gloves be worn contact with the refrigerant can cause blindness and other physical injuries to the operator.
- Avoid contact with the skin the low boiling point of the refrigerant (approx. 30 °C) can cause frost burns.
- Avoid inhalation of vapours from refrigerants.
- Ensure that all the valves are closed before making connections between the unit and an A/C system or an external tank.
- Ensure that the phase has been completed and that all valves are closed before disconnecting the unit. This will prevent release of the refrigerant into the atmosphere.
- Do not modify the safety valve or control system settings.
- Do not use external tanks or storage containers that have not been type-approved or that are not fitted with safety valves.
- Do not leave the unit connected to a power supply unless it is going to be used immediately. Switch off the electrical power supply if the unit is to be out of use for prolonged periods.
- All of the flexible hoses may contain refrigerant at high pressure.
- Disconnect flexible hoses with extreme caution.
- The service unit and A/C systems in vehicles containing refrigerants should not be tested with compressed air. Some mixtures of air and refrigerant have proven to be combustible at high pressure levels. These mixtures are potentially hazardous and there is a risk of fire and explosions that can cause damage to property and personal injury.
- Additional medical and safety information can be obtained from the manufacturers of the lubricants and refrigerants used.
- Remember that the unit must be supervised at all times.
- The unit **must not** be used in potentially explosive environments.
- Do not smoke near the unit



5.1.1 Special instructions for units to be used with R-1234yf

- Refrigerant R-1234yf is an inflammable gas.
- When using the unit, check that the fan close to the non-condensable gas discharge is operating.
- When using the unit, connect a dedicated discharge gas evacuation system to the noncondensable gas discharge flange.

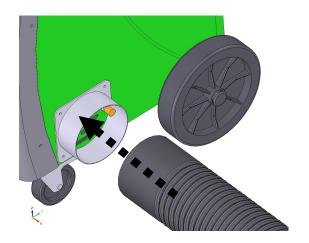



5.2 Guidelines for handling refrigerants

5.2.1 Glossary of terms

- **Refrigerant:** A refrigerant fluid solely of the type for which the unit has been designed (check on the identification plate located near the main switch of the unit).
- A/C system: Air conditioning system in the vehicle.
- **Unit:** *ICEGARD BLU* equipment for the recovery, recycling, vacuum and filling of the A/C system.
- Operator: qualified person able to use the unit
- External tank: New, non-refillable refrigerant cylinder, used to fill the internal container.
- Internal container: Refrigerant storage tank.
- **Phase:** Execution of an individual function.
- Cycle: Execution of each individual phase in sequence.
- **Recovery:** The removal of refrigerant in any condition and its storage in a container outside the A/C system, without necessarily undergoing analysis or treatment of any kind.
- **Recycling:** A reduction in the contaminating substances in used refrigerants through oil separation, the removal of un-condensable gases and their single or multiple passage through elements that enable a reduction in humidity, acidity and particles.
- **Disposal:** Removal of refrigerant to storage, for subsequent destruction or transfer to disposal centres.
- **Vacuum:** Phase in which un-condensable gases and moisture are evacuated from an A/C system solely by means of a vacuum pump.
- Oil injection: Introduction of oil into an A/C system for the purpose of maintaining the correct amount specified by the manufacturer.
- **UV additive injection:** Introduction of UV additive into an A/C system to detect any leaks in the A/C system.
- **Filling:** Phase in which refrigerant is introduced into an A/C system in the amount specified by the manufacturer.
- **Flushing**: A\C system cleaning phase from any contaminants by circulation of refrigerant.
- Lake test with Nitrogen: filling A/C system with nitrogen in order to detect leakages for pressure decay
- **Un-condensable gases:** Air accumulated during the refrigerant vaporizing phase, extracted from A/C systems or tanks.




5.2.2 Precautions for refrigerant storage

Refrigerant to be removed from a system must be handled carefully in order to prevent or minimise the possibility of mixing different refrigerants.

The unit is specifically designed for the treatment of only one type of refrigerant, check it on the identification plate.

The cylinders used for storing refrigerants must be assigned to specific refrigerants to avoid mixing refrigerants of different types.

The cylinders used must be free of oil and other contaminants and must be clearly marked in order to identify the refrigerants they contain.

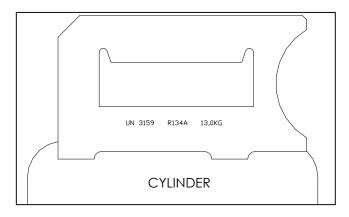

5.2.3 Condition of the refrigerant and the system

The history and age of a system can be important factors in deciding whether or not to recycle its refrigerant.

Installation and maintenance procedures carried out during the system's service life have a significant effect on the quality of the refrigerant.

Systems that have not been cleaned or properly evacuated may have high levels of contamination in the refrigerant and the oil. If the system's history is unknown, the refrigerant removed must at least be recycled before being re-introduced into the system.

When operators are unsure of the level of the refrigerant's contamination, preliminary checks can be performed using special kits for measuring acidity and humidity.

5.2.4 Recycling capacity

The recycling unit's filter systems must be replaced regularly (Chap. MESSAGES) in order to maintain the efficiency of the recycling unit.

However, even if all factors indicate that recycling of the refrigerant is not necessary, recycling should nevertheless be carried out.

5.2.5 General considerations

Before re-introducing refrigerant into the system, the system itself must be evacuated and cleaned. In order to be sure that the system is free of contaminating agents, all the procedures described in this manual must be followed before introducing the refrigerant.

Clean and maintain the units regularly, especially when highly contaminated refrigerant has been used: it is extremely important that contamination from the previous servicing operation is not transferred to subsequent operations.



5.3 Safety devices

The ICEGARD BLU is equipped with the following safety devices:

- Safety pressure switch: Stops the compressor in the event of excessive pressure.
- Safety valve.



No tampering with the above-mentioned safety devices is permitted.

5.4 Working environment

- Working environment must be compliant with the national laws.
- The unit must be used in an open or well-ventilated environment (at least 4 changes of air per hour).
- The unit has been designed for use at a maximum altitude of 1000 m above sea level, within a temperature range of +5 °C to +50°C and with maximum humidity of 50% at +40 °C.
- Work in a well-lit environment (the average illumination value for work in mechanical and assembly workshops (for precision work) is 500 750 1000 lux).
- Work well clear of naked lights, sparks and hot surfaces. At high temperatures, the
 refrigerant breaks down, releasing toxic and chemical substances that are harmful to
 operators and the environment.
- Avoid inhaling the refrigerants and oils in the systems. Exposure may cause irritation to eyes and the respiratory tract.



6 USE

6.1 Unpacking and checking the components

Remove the unit's packaging.

Check that all of the accessory components are present:

- Instruction manual
- 2 cylinder connectors
- Power cable
- Safety kit (gloves, goggles)

6.2 Unit handling and storage

Remove the unit from the base pallet of the packaging. The unit is moved on all four wheels. The two front wheels have brakes.




Although the heaviest components have been assembled on the base in order to lower the centre of gravity, it has not been possible to totally eliminate the *risk of overturning*.

For transport of the unit or its handling over long distances or on rough surfaces, place the inner container in the safety position for transport purposes.

Replace the inner container in the working position before operating the unit.

- Safety position for transport purposes. Tighten the support screws to the end of the stroke. Do not force it when it has reached the end of the stroke.
- **Working position.** Loosen the support screws to the end of the stroke. Do not force it when it has reached the end of the stroke.

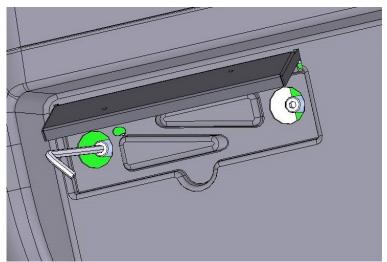



Turn the screws alternately to move the inner container in a vertical position.




6.3 Preparation for use

Once the unit has been moved close to the air conditioning system to be serviced, make sure it is resting on all four wheels on a flat, horizontal surface and locked wheels with brake in order to ensure proper functioning of the scales.

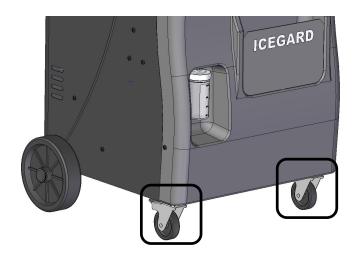




The unit must then be connected to a main supply that conforms to what is indicated on its identification plate (located next to the ON/OFF switch) especially with regard to **voltage**, **frequency and applicable power**.

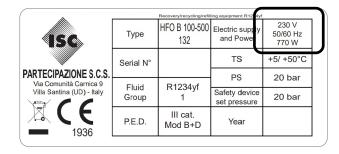



6.4 Start-up

Place the Unit on an horizontal position with oil and uv empty containers Connect the unit to the main supply, move the ON/OFF switch (42) to the ON (I) position.

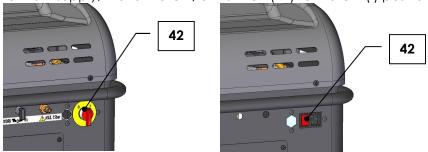

When the Unit is switched on for the first time, it is necessary to select the language among the available ones; the language proposed is Italian.

SELECT LANGUAGE English

Enter-Ok Stop-Exit

Press **UP** and **DOWN** to select the requested language. Confirm with **ENTER**. Then the unit performs automatically the pressure sensor calibration.

Vacuum in progress
XX

The unit performs a vacuum phase.

Calibration ok!

If at the start up new software is detected in the USB memory stick (if placed), the upgrade is performed automatically.

If previously had been

set the POE "hybrid" oil

settings the display will show the corresponding message.

Press **ENTER** to confirm.

Display shows for a few seconds the name of the unit, the software version installed and then the oil type settings (see paragraph 12.3 kit POE "Hybrid").

ICEGARD BLU

SW xx xx xx xx

Oil type settings PAG

Enter-OK

Press **ENTER** to confirm.

The display will then show the available resources (stand by):

Available refrigerant g xxx

Enter-OK

Only now is possible lower the inner container. Ref. Subsection 6.2 Unit handling and storage



6.5 Switching Off

To switch the unit off, move the main switch (42) to the OFF (0) position.

6.6 Internal tank filling phase



FOLLOW CAREFULLY THE INSTRUCTIONS BELOW TO PREVENT RELEASE OF THE REFRIGERANT INTO THE ATMOSPHERE

There are two types of source tank: with dip tube and without dip tube:

- With dip tube,
- Without a dip tube.

Tanks **with dip tube** must remain upright in order to be able to transfer the liquid refrigerant. Use connection **L** (liquid) for this type of tank.

Tanks **without a dip tube** have one valve only. They must therefore be turned upside down in order to transfer the liquid refrigerant.

Types of tank





Tank with dip

Tank without dip

Open the **HP** valve on the control panel. Press the **ENTER** key in stand-by mode.

Car/customer data	
Skip data	
Other menus	
Enter-Ok Stop-Exit	

Press the **UP** and **DOWN** keys to select **Other menus**. Confirm with **ENTER** key.

Int. tank filling ■
Service □
Print □
Enter-Ok Stop-Exit

The **Print** menu is visualized only if they are present on the unity the printer. Press the **UP – DOWN** keys to select **Int tank filling**. Confirm with **ENTER** key.

Connect HP hose to the external tank. Open the tank valve Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with **ENTER** key.



Enter the required quantity and confirm g. Enter-Ok Stop-Exit

Enter the quantity to load inside the tank with the **UP – DOWN** keys. Confirm with **ENTER** key.

Please wait !

Stop-Exit

Filling in progress recovered quantity g. Stop-Exit

Required quantity ok Close the external tank valve Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with **ENTER** key.

Attendere ! Recupero Refrigerante dai Tubi di servizio Stop-Exit

Fasi completate.

Enter-Ok


Confirm with **ENTER** key. The display visualizes the stand-by mode.


The maximum refrigerant quantity storable inside the internal container is 10 Kg (38kg HD). Consider that after the message "Close the external tank valve" the unit could still recover almost 1 kg.



6.7 Draining of incondensable gases

The non-condensable gas drain valve (33) is installed to allow gradual evacuation of the non-condensable gases in the internal tank.

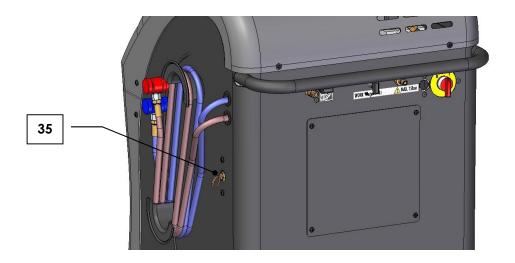

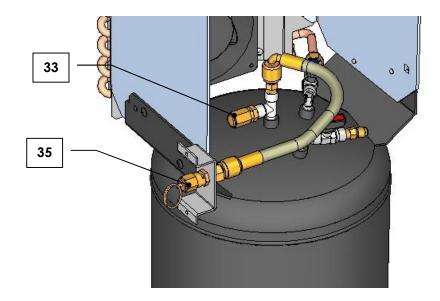

It operates **automatically** whenever non-condensable gases are present inside the non-condensable tank and their pressure exceeds the set pressure.

The purpose of the non-condensable gas discharge valve (33) is to allow gradual evacuation of non-condensable gases present inside the internal tank once they exceed the set pressure.



7 MESSAGES

7.1 Malfunction/error messages

Chassis evacuation.
Please wait.
Poor Ventilation
RPM xxxx

This message appears only with the version for R-1234yf. Chassis air flow not sufficient. The unit can't be used till ventilation rehabilitated. Contact your distributor.

Warning! Over-pressure in internal tank Stop-Exit

Overpressure in internal container. Wait about 30 minutes and then re-run the recovery/recycling function. Call Customer Service if the problem persists.

Tank hanged or weight scale calibration wrong Stop-Exit

Attempt to perform a recover/recycling phase or filling of inner tank with the gas bottle in the safety position for transport purposes. Place the inner container in the working position. The message may also be displayed in the presence of incorrect calibration of the refrigerant scales.

Warning! Internal tank filled. Stop-Exit

Absolute maximum permitted weight of refrigerant in internal container reached. This value should never be exceeded under any circumstances.

Warning!
pressure inside the
A/C system.
Recycling start.

Appears <u>at the start</u> of the vacuum phase if pressure is found in the A/C system. The unity performs a recycling phase.



A/C system leakage Continue? mB. Enter-Ok Stop-Exit

A/C system not sealed. This message appears if an increase in the pressure reading occurs during the leakage check. Repair the A/C system. Press the **ENTER** Key to proceed with the next phase. Press the **STOP/BACK** key to return to stand-by mode.

Insufficient vacuum Continue?

mb.
Enter-Ok Stop-Exit

 Appears after a vacuum time of 10 minutes if the pressure in the A/C system has not dropped below 100 mBar.

Press the **ENTER** Key to continue the vacuum phase. Press the **STOP/BACK** key to return to stand-by mode.

Warning! Insufficient vacuum.

Enter-Ok Stop-Exit

Overpressure during the pressure check phase at the beginning of the oil injection or UV additive injection phases. This phase is only carried out on A/C systems currently under vacuum. Pres **ENTER** to confirm. Press the **STOP/BACK** key to return to stand-by mode.

Refr. qty. insuff. Perform int. tank Filling phase? Enter-Ok Stop-Exit

Too low refrigerant quantity inside the internal tank. Press **ENTER** to make a recovery phase from external tank. Press **STOP/BACK** to visualize the next step.

External tank empty or valve closed! Check Enter-Ok Stop-Exit

Appears at the start of the internal tank filling phase if there is no pressure or during the phase if the quantity of refrigerant set has not been reached.

Empty out drained oil container

Enter-Ok Stop-Exit

Appears at the start of the recycling phase or during the oil discharge phase



Exceeding recycling time Continue? Enter-Ok Stop-Exit

The maximum time allowed for the recovery/recycling phase has been reached. Check the pressure values on the gauges. If there is pressure, there may be a fault in the unit (call Customer Service). If there is no pressure, there may either be a leak in the A/C system or in the solenoid valves. Press the **ENTER** key to continue the recovery/recycling phase. Press the **STOP/BACK** key to return to stand-by mode.

Exceeding filling time Continue? Enter-Ok Stop-Exit

Turn HP connector gear counterclockwise Enter-Ok

Start A/C system

Enter-Ok

Open LP Valve

Enter-OK

Appears during the filling phase if the set quantity has not been reached during the maximum planned time if a **HP-LP** A/C system has been selected.

The remaining quantity of refrigerant is sucked by the compressor of the A/C system by following the instructions shown on the display. Following the instruction and than press **ENTER** to continue the filling phase. Press the **STOP/BACK** key to return to stand-by mode.

Exceeding filling time Continue? Enter-Ok Stop-Exit

Appears during the filling phase if the set quantity has not been reached during the maximum planned time if only a **HP** A/C system has been selected.

Press the **ENTER** key to continue the filling phase. Press the **STOP/BACK** key to return to stand-by mode.

Exceeding filling time

Enter-Ok

Press the **ENTER** key to continue.



Start A/C system

Enter-Ok

Appears during the filling phase if the set quantity has not been reached during the maximum planned time if only a **LP** A/C system has been selected.

The remaining quantity of refrigerant is sucked by the compressor of the A/C system by following the instructions shown on the display.

usb card not found Insert usb card Enter-Ok Stop-Exit

Appears if the memory stick is not found when exporting, the following message appears check the presence, operation and correct installation of the memory stick.

File
Back up
Not found
Enter-Ok Stop-Exit

Appears if the memory stick is not found during the data restore, the following message appears check the presence, operation and correct installation of the memory stick.

7.2 Function messages

Oil type settings PAG

Enter OK

Appear at the start up to indicate that the type oil settings are currently on PAG mode. Confirm with **ENTER** key.

Oil type settings POE "Hybrid"

Enter OK

Appear at the start up to indicate that the type oil settings are currently on POE "hybrid mode. Confirm with **ENTER** key.

Replace filter Recycling and vacuum pump oil. Enter-Ok

Appear at start-up if unit requires programmed maintenance. Reset respective work counters after replacing components. See paragraph 11.4.3 Counters reset.

Sensor pressure



Confirm start
selected phases?

Enter-Ok Stop-Exit

Press the **ENTER** key, the unit performs the phases or the programmed cycle.

Process completed

Enter OK

Press the **ENTER** key, the display shows the stand-by mode.

Available new data base version

Enter OK

Appear after one year from the first activation of the unit if the memory card is present. Press the **ENTER** key.

Please contact your dealer

Enter OK

Appears after one year from the first activation of the unit. Press the **ENTER** key, the display shows the stand-by mode.

Insert a memory stick in the USB port with a new version of the data base and switch ON the unit. Enter the password in order to update the data base.

Printer not available Continue? Enter-Ok



Printer not on line (printer LED flashing). Possible causes are printer lid not closed or lack of paper. Press the **ENTER** key to proceed with the next phase. Press the **STOP/BACK** key, the display shows the stand-by mode.

If the paper has finished, lift the printer lid to prevent print head from burning.



Only use ISC Systems paper.

The appearance of one of these messages is accompanied by a buzzer sounding. Press ENTER key to go out.



8 OPERATING DESCRIPTION

With the unity on stand-by mode, display shows the available refrigerant.

8.1 Operating Modalities

The Unit memorizes the set values concerning the services performed on the A/C plants on the basis of the plate number if an automatic program, or a filling phase, has been carried on; setting a plate number already existing in the unit memory, it is possible to view the previous service data and to repeat the same service.

The Unit is able to operate also in the following cases:

• Automatic program:

It is possible to select a user models previously saved or set the charge refrigerant quantity. The automatic program calculates the vacuum time according to the refrigerant quantity set.

User program:

the User can select which phases he wants to perform.

After the selection of the preferred program, follow the instruction showed on the display.

From the automatic program you can also select a specific car model from a data base; furthermore a diagnosis system is present and it is able to check the performances of the A/C systems indicating the possible causes of unsatisfactory results.

8.2 Modality of programming

- Press UP and DOWN keys to select the desired program.
- Press ENTER key to confirm the selection.
- Press STOP/BACK key to interrupt the function execution and come back on stand-by.
 Press STOP/BACK key to come back to previous screening during settings.



8.3 Editing

During the phase of insertion plate number, with any character shown to display, pressing the **ENTER** key he passes to screens it following.


Pressing the **UP** key he departs from the letter A and they is flowed the characters in hourly sense.

Pressing the **DOWN** key he departs from the number 9 and they is flowed the characters in clockwise sense.

Pressing the **ENTER** key he goes to next digit.

Pressing the STOP/BACK key he returns to the preceding digit.

Pressing the **ENTER key for 3 seconds** the introduced datum is confirmed.

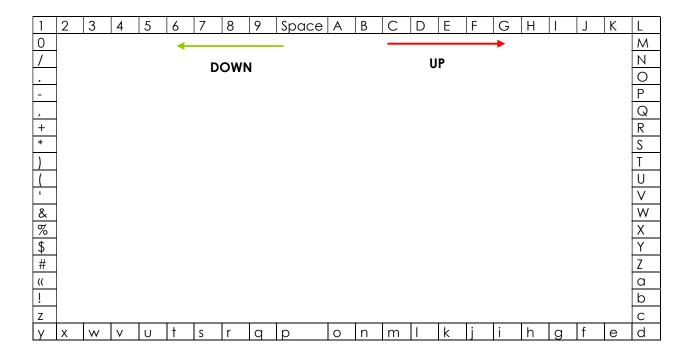



9 PROGRAMS

Connect the **LP-HP** connectors (or the single connector) to the A/C system. Open the connectors (or the single connector) by turning the knob clockwise. The **LP-HP** gauges (or the single pressure gauge) indicate the pressure in the two branches of the A/C system.

Press the **ENTER** key with the display in stand-by mode.

a.,,.	The software is upgraded frequently, it is possible							
Set plate number ■ Skip data □			differences					
_	manual.							
Enter-Ok Stop-Exit								

Press the **UP** and **DOWN** keys to select the desired menu. Confirm with **ENTER** key.

Plate number

If you do not want to insert the plate number press **ENTER** key. Insert the plate number with **UP – DOWN** keys. See paragraph **8.3 Editing.** Confirm the plate number pressing **ENTER for 3 seconds**.

9.1 Recognition developed services

In case the Unit finds that a service has been performed previously with reference to the same number plate introduced by the User, the display shows the following info.

Plate no.
Perform as prev.

Prev. service data □
Enter-Ok Stop-Exit

- Select PERFORM AS PREVIOUS and press ENTER key to confirm for service start.
- Select DATA PREVIOUS SERVICE and press ENTER key to view the recorded data.

Press **UP** and **DOWN** keys to scroll the following information:

- Filled quantity
- Vacuum time
- Leak test time
- Pressure increase during leak test time
- Oil injected? Yes/No
- UV injected? Yes/No
- Refrigerant recovered quantity



Press **ENTER** key to confirm the service. See paragraph **10 START OF PROGRAMMED CYCLES**. Press **STOP/BACK** key to program the service again.

If any service is not found inside the memory of the unity for the same number of plate, or if you chose to program the service again, the display shows:

HP/LP couplers	
HP coupler only	
LP coupler only	
Enter-Ok Stop-Exi	t

Press **UP - DOWN** to select. Confirm with **ENTER**. See paragraph:

- 9.2 Automatic Program,
- 9.3 User Program.

9.2 Automatic Program

You have access to following screen after having performed the operations brought in the paragraph **9 PROGRAMS**.

Automatic program □ User program □
Enter-Ok Stop-Exit
Press UP - DOWN to select. Confirm with ENTER key.
Enter filling value ■ User models
Enter-Ok Stop-Exit
Press UP - DOWN to select. Confirm with ENTER key.
Enter the quantity g XXXX
Enter-Ok Stop-Exit

Insert the correct refrigerant value with the **UP - DOWN** key and confirm with **ENTER** key.

Refr. q.ty g XXXXX Vacuum time XX:XX

Confirm with **ENTER** key.

The vacuum time is calculated in comparison to the filled refrigerant quantity.

Press the **UP** or **DOWN** keys to access the programming of injection oil – UV phases. See paragraph **9.4 Programming injection oil-UV phase**.

Press **ENTER** key for next step.



Iso Oil	46	
	100	
	150	
Enter-Ok	Stop-	-Exit

Press the **UP** and **DOWN** keys to select the oil. Confirm with **ENTER** key.

Pressing the **ENTER** key the automatic cycle starts with the inserted data and manual injection oil-UV.

9.2.1 Model Search (Data base)

Select Search models to have access to vehicles data base.

Enter required q.ty □
Search models ■

Press the **UP** and **DOWN** keys to select the desired menu. Confirm with **ENTER** key.

User Models
> Alfa Romeo <
 Audi
Enter-Ok Stop-Exit</pre>

Press **UP** and **DOWN** Key to select the brand desired or to access to the **User models**. Confirm with **ENTER** key.

Selecting the brand desired You have to repeat the same operation for all the requested fields of application in order to identify the exact quantity to fill.

Refr. q.ty g XXXXX Vacuum time XX:XX

The vacuum time is calculated in comparison to the inserted refrigerant quantity. Confirm with **ENTER** key.

Iso Oil 46 ■ 100 □ 150 □ Enter-Ok Stop-Exit

Press the **UP** and **DOWN** keys to select the oil. Confirm with **ENTER** key.

Pressing the **ENTER** key the automatic cycle starts with the inserted data and manual oil - UV injection.



9.2.2 User models

> User Models < Alfa Romeo Audi Enter-Ok Stop-Exit

Press **UP** and **DOWN** Key to select the **User models.**

> User Model 1 <
 User Model 2
Enter-Ok Stop-Exit</pre>

Press **UP - DOWN** to select the user model that you desired. Confirm with **ENTER** key. If the selected model had already been planned; the display shows the saved data:

Refr. q.ty g XXXXX Vacuum time XX:XX

Press the **UP** or **DOWN** keys to access the programming of injection Oil – UV phases.

See paragraph 9.4 Programming injection oil-UV phase.

Pressing the **ENTER** key the automatic cycle starts with the inserted data and manual oil – UV injection.

The data previously inserted can be modified pressing **ENTER for 3 seconds** during the data screening.

To set the data of a new user model, place yourself on a free user model and press **ENTER** key. The display shows:

Mod.:

Refrigerant q.ty. g

Vacuum time:

Enter-Ok Stop-Exit

On the display blink the model name

Insert the name of the user model with **UP** and **DOWN** keys.

See paragraph 8.3 Editing.

Confirm the name of the model pressing **ENTER**.

On the display blink the refrigerant quantity.

Set with **UP** and **DOWN** keys then confirm pressing **ENTER**.

On the display blink the vacuum time.

Set with **UP** and **DOWN** keys then confirm pressing **ENTER**.

On the display blink one more time the model name

If the data are set confirm pressing ENTER for 3 seconds

You come back to screen which shows You the choice of the user models.



9.3 User Program

You	access	to	following	screen	after	having	performed	the	operation	brought	in	the	parag	graph
9.Pro	grams,	the	e display sh	nows:										

Automatic program	
User program	
Enter-Ok Stop-Exit	

Press the **UP** and **DOWN** keys to select the desired menu. Confirm with **ENTER** key.

Recycling? Yes
No
Enter-Ok Stop-Exit

Press the **UP** and **DOWN** keys to select. Confirm with **ENTER** key. If **NO** option is selected, the display proposes the **vacuum phase**. If **Yes** is selected, the display shows:

Recycling? YES
Pressure increase
test time min. x
Enter-Ok Stop-Exit

The display proposes 1 minute pressure increase control before finally completing the refrigerant recovery phase. Set the desired value with **UP – DOWN** keys. Confirm with **ENTER** key.

Vacuum phase yes no Enter-Ok Stop-Exit

Press the **UP** and **DOWN** keys to select. Confirm with **ENTER** key. If **NO** is selected, the display proposes the **charging phase**. If **Yes** is selected, the display shows:

Vacuum time 20
Leak test
time min. 4
Enter-Ok Stop-Exit

The display proposes a 20 minutes vacuum phase; set the desired value with **UP – DOWN** keys. Confirm with **ENTER** key.

The display proposes a 4 minute leakage control at the end of the vacuum time. Set the desired value with **UP – DOWN** keys. Confirm with **ENTER** key.

Oil-UV injection? Yes
No
Enter-Ok Stop-Exit

Press the **UP** and **DOWN** keys to select. Confirm with **ENTER** key. If **NO** is selected, the display proposes the **charging phase**.



If **Yes** is selected, the display shows:

Automatic Oil-UV	
Manual Oil-UV	
Timed Oil-Uv	
Enter-Ok Stop-Exi	t

Press the **UP** and **DOWN** keys to select. Confirm with **ENTER** key.

If automatic Oil – Uv is selected, the display proposes the programming phase of automatic oil-UV injection. See paragraph **9.4.1 Automatic Oil - UV injection**.

If Timed Oil – Uv is selected, the display proposes the programming phase of Timed oil-UV injection. See paragraph **9.4.3 Timed Oil – Uv injection**.

If **Manual Oil-Uv** is selected the diplay proposes:

```
Filling phase
Enter quantity
g. 700
Enter-Ok Stop-Exit
```

Set the quantity of refrigerant to be filled with **UP** and **DOWN** keys. Confirm with **ENTER** key.



Confirm start selected phases?

Enter-Ok Stop-Exit

Confirm with ENTER key.

9.4 Programming injection oil-UV phase

9.4.1 Automatic Oil - UV injection

Automatic Oil-UV	
Manual Oil-UV	
Timed Oil-Uv	
Enter-Ok Stop-Exi	t

Press the **UP** and **DOWN** keys to select **Automatic Oil-UV**. Confirm with **ENTER** key.

```
Iso Oil 46 ■
100 □
150 □
Enter-Ok Stop-Exit
```

Press the **UP** and **DOWN** keys to select the oil. Confirm with **ENTER** key.

After the vacuum phase the unit inject 10g of oil more then the quantity of drained oil during recovery phase.

```
UV timed Yes injection? No Enter-Ok Stop-Exit
```

Press the **UP** and **DOWN** keys to select. Confirm with **ENTER** key.

If **NO** is selected, the display proposes the next phase.

If **YES** is selected, the display proposes:

```
UV quantity g 5

Enter-Ok Stop-Exit
```

Set the quantity of UV to inject with the **UP** and **DOWN** keys. Confirm with **ENTER** key. The unit proceed to the next phase



9.4.2 Manual Oil - UV injection

	Automatic Oil-UV Manual Oil-UV Timed Oil-Uv Enter-Ok Stop-Exit	
	Press the UP and DOWN keys to select Manual Oil-UV . Confirm with ENTER key. After the vacuum phase the unit will stop in order to make the manual oil – UV injection.	
	9.4.3 Timed Oil – Uv injection	
	Automatic Oil-UV Manual Oil-UV Timed Oil-Uv Enter-Ok Stop-Exit	
	Press the UP and DOWN keys to select Timed Oil-Uv injection. Confirm with ENTER key.	
	Iso Oil 46 ■ 100 □ 150 □	
l	Enter-Ok Stop-Exit	
	Press the UP and DOWN keys to select the type of ISO oil. Confirm with ENTER key.	
	Oil quantity g 510	
	Enter-Ok Stop-Exit	
	Set the quantity of oil to inject with the UP and DOWN keys. Confirm with ENTER key.	
I	UV timed Yes injection? No	
	Enter-Ok Stop-Exit	
	Press the UP and DOWN keys to select. Confirm with ENTER key. If NO is selected, the display proposes the next phase. If YES is selected, the display proposes:	
I	UV quantity g 5	
	Enter-Ok Stop-Exit	
	Set the quantity of Uv to inject with the UP and DOWN keys. Confirm with ENTER key. The display propose the next phase.	





Warning: visually check that the quantity of oil and UV, in their containers, are sufficient to perform the required injection procedure.



Timed injection will be carried out with a precision of \pm 15 g (at room temperature between 20 and 30°).

In case of timed injection, modification of the quantity of oil to be injected will still be possible during performance of the vacuum phase.

Press the **ENTER** Key for 3 seconds; the display shows the previously set quantity of oil to be injected. Use the **UP - DOWN** keys to program the quantity of oil to be injected into the A/C system. Confirm with the **ENTER** Key.

The display shows the remaining time for the vacuum phase.



10 START OF PROGRAMMED CYCLES

Open the LP and HP valves on the control panel, or the single valve, according to the type of A/C system selected.

10.1 Recovery/recycling phase

Please wait!

Stop-Exit

This message appears on the display for few seconds.

Recycl. in progress recovered quantity Stop-Exit

When the unit detects that the A/C system is empty, the function stops automatically. A check on the pressure increase inside the A/C system is started

Pressure increase Test.

Sec.

Stop-Exit

If the pressure in the A/C system rises up, the recovery phase starts again automatically.

Check drained oil quantity.

Quantity g.

The unit drains the extracted oil into the oil drain container (21).

Please wait!

Stop-Exit

Recycling completed Recovered quantity

The recovery/recycling phase is now completed.



10.2 Vacuum phase

Vacuum	in	progress.
Time		xx:xx
Stop-Ex	it	

When the time is expired, the control of any leakages in the A/C system starts.

```
Leak test in
Progress sec.
mb xx
Stop-Exit
```

The data is shown on the display for a few seconds.

Vacuum completed mb.

If the **timed Oil - UV injection** and the **LP** and **HP** hoses were chosen; at the end of vacuum phase on the diplay appears:

Close LP Valve

Enter OK

Follow the instructions. Confirm with ENTER key.

If the **ENTER** key is not pressed, at the end of the vacuum phase, the unit stops and the message appears again.



10.3 Oil – UV injection

10.3.1 Automatic Oil – UV injection

Oil injection in progress

Stop-EXIT

This message appears during the oil injection.

Oil injection Completed

Stop-EXIT

This message appear at the end of oil injection, the unit automatically proceeds to the next phase.

UV timed injection in progress Stop-EXIT

This message appear during the UV injection

UV timed injection completed Stop-EXIT

This message appears at the end of UV injection. The unit automatically proceeds to the charging phase.

10.3.2 Timed Oil – UV injection

Oil injection in progress

Stop-EXIT

This message appears during the oil injection.

Oil injection Completed

Stop-EXIT

This message appear at the end of oil injection, the unit automatically proceeds to the next phase.



UV timed injection in progress Stop-EXIT

This message appear during the UV injection.

UV timed injection completed Stop-EXIT

This message appears at the end of UV injection.

The unit automatically proceeds to the charging phase.

10.3.3 Manual Oil – UV injection

Oil inject

Enter-Ok Stop-Exit

Visually check that the quantity of oil in the oil injection container is sufficient to perform the required injection procedure.

Press and keep the **ENTER** key pressed to perform the oil injection.

To finished oil injection release ENTER key and press STOP/BACK key.

Press **STOP/BACK** key to skip the oil injection.

The unit proceeds to the UV manual injection.

UV injection

Enter-Ok Stop-Exit

Check visually that the quantity of UV in the UV injection container is sufficient to perform the required injection procedure.

Press and to maintain pressed the **ENTER** key to effect the UV injection.

To complete UV injection release ENTER key and press STOP/BACK key.

Press STOP/BACK if You do not want to perform UV filling.

The unit proceeds automatically to refrigerant charging phase.



10.4 Charging phase

The unit stops before making the charging phase only if been chosen **LP** and **HP** hoses and **Oil – UV manual injection**; the display shows the following messages:

Close LP valve

Enter-OK

Follow the instructions and than press ENTER key.

Filling phase in progress quantity g. Stop-Exit

The data are visualized during the charging phase.

Filling completed. Quantity g.

Process completed

Enter-Ok

Press **ENTER** to confirm.

phase is performed intermittently.

Working on only LP

plants, the filling

port

If the pressure of internal tank is not enough to complete the filling phase, a procedure to fill the remaining quantity with the suction port of the A/C system compressor is carried out.

See Paragraph 7 MESSAGES.

If the memory card is present, after the charged phase can be accessed at diagnosis of the A/C system by the following screen:

A/C system Yes diagnosis? No

Enter-OK

If Yes is selected You access to diagnosis of the A/C system. See section 11.2 Diagnosis.

P.S. Even without the diagnosis installed we suggest to check A/C system performance. Close **LP – HP** valves. Start the engine and keep it around 1.500/2000 r.p.m. Start the A/C system. Reduce the A/C temperature to a minimum and increase the ventilation speed to the maximum. Wait until the stabilization of the A/C system. Check the pressure on the manometers and the temperature at the central blower. Turn off the A/C system and the engine.



If **No** is selected the display visualize:

Disconnect HP/LP hoses from A/C ENTER-OK STOP-EXIT

Keep the Unit isolated from the A/C System.

Open **LP** and **HP** valves. Confirm with **ENTER** key.

WAIT! Refrigerant recovery from HP/LP hoses Stop-Exit

The unit performs the recovery from the hoses.

Close LP and HP Valves

Enter-OK

Follow the instructions and than press ENTER. The display shows the stand-by mode.

11 OTHER MENUS

Press the **ENTER** key with the display in stand-by mode.

Set plate number ☐
Skip data ☐
Other menus ■
Enter-Ok Stop-Exit

Press the **UP** and **DOWN** keys to select the **Other menus**. Confirm with **ENTER** key.

Int.tank filling
Service
Print
Enter-Ok Stop-Exit

Diagnosis
Gas Analyzer
Back up/restore
Enter-Ok Stop-Exit

Print menu is displayed only if they are present in the Unit the printer. Press the **UP** and **DOWN** keys to select the desired menu. Confirm with **ENTER** key.

11.1 Filling internal tanks

See paragraph 6.6 Internal tank filling phase.



11.2 Diagnosis

The unit is equipped with a diagnosis system and it is able to check the performances of the A/C systems indicating the possible causes of unsatisfactory results.

The appropriate function of A/C diagnosis is available both at the end of filling phase and from **Other menus**.

Close LP and HP Valves Enter-OK

Follow the instructions. Confirm with **ENTER** key.

The display shows the following only if you access to diagnosis from Other menus.

Connect HP/LP hoses to the A/C system Enter-OK Stop-Exit

Follow the instructions. Confirm with ENTER key.

Start A/C for checking

Enter-OK

To perform a diagnosis in the correct way start the engine and keep it around 1.500/2000 r.p.m. Reduce the A/C temperature to a minimum and increase the ventilation speed to the maximum. Let the A/C System running for 10 minutes

Follow the instructions. Confirm with **ENTER** key.

Check the values reported here below:

- **T.E** external temperature, (C°)
- T.I internal temperature at the main small opening of the A/C,
- **P.HP** pressure detected by the manometer HP, (bar)
- **P.LP** pressure detected by the manometer LP, (bar)

A/C system diagnosis P.HP: P.LP: . T.I.: T.E.: . Enter-Ok Stop-Exit



- **-(V.)** only for **variable** displacement compressor.
- **-(F.)** only for **fixed** displacement compressor.

Insert the required values through the **UP** and **DOWN** keys. Confirm with **ENTER** key after each data entered. When all the values are entered, confirm with **ENTER** key for 3 seconds.

The unit elaborates the data. In case of not reasonable data or unsatisfactory performances, the display shows the different situations that may occur in the A/C system. Each case is indicated with single screen.

Example of diagnosis screen:



Compressor hoses reversed Enter-Ok

Press **UP** and **DOWN** key for showing the next cases. Press **ENTER** key to continue.

11.2.1 Hoses empting

Disconnect HP/LP hoses from A/C

ENTER-OK

Keep the Unit isolated from the A/C System.

Confirm with ENTER key.

Open LP/HP Valves

Enter-OK

Follow the instructions. Confirm with ENTER key.

WAIT! Refrigerant recovery from HP/LP hoses Stop-Exit

The Unit recovers the refrigerant or the vapours of refrigerant still present inside the charging hoses. The display shows:

Close LP/HP Valves

Enter-OK

Follow the instructions. Confirm with **ENTER** key. The Unit shows the stand-by mode.



11.2.2 Suction of refrigerant through the A/C System

Selecting the diagnosis from **Other menus**, at the end of the diagnostic phase, the unit carries out the procedure to let the A/C systems recovering the refrigerant present inside the charging hoses.

Disconnect HP hose from A/C system

Enter-Ok

Follow the instructions. Confirm with ENTER key.

Open LP/HP Valves

Enter-OK

Follow the instructions. Confirm with **ENTER** key.

Wait till when the compressor of the A/C system recovers the refrigerant contained in the **HP/LP** hoses. When the pressure detected with the manometers stops to decrease press **ENTER** Key.

Switch off A/C system

Enter-OK

Follow the instructions. Confirm with ENTER key.

Disconnect LP hose from A/C system

Enter-OK

Follow the instructions. Confirm with ENTER key.

WAIT! Refrigerant recovery from HP/LP hoses Stop-Exit

The unit recovers the refrigerant or the vapours still present in the hoses. The display shows:

Close LP/HP Valves

Enter-OK

Follow the instructions. Confirm with **ENTER** key. The display shows the stand by mode.



11.3 PRINTER

This menu is visualized in **Other menu** only if the printer is installed.

The **ICEGARD BLU**, with printer, prints a coupon which reports the info concerning each service phase performed; the functions specified here below are also available:

Repeat print Customize data	
ENTER-OK STOP-EXIT	

Press the **UP** and **DOWN** keys to select the desired menu. Confirm with **ENTER** key.

11.3.1 Repeat service report

Select **Repeat print** to print a copy of the service report of the last service performed.

11.3.2 Personalization of service report heading

Select **Customize data** to modify the heading of service report.

The heading is composed of 5 lines and 20 characters.

Repeat print Customize data	
ENTER-OK STOP-EXIT	

Press the **UP** and **DOWN** keys to select the desired menu. Confirm with **ENTER** key. The display shows the following screen:

Enter company data ISC Systems Enter-Ok Stop-Exit

You can change one line at a time, select the line to be changed with the **UP** and **DOWN** keys. Confirm with **ENTER** key. The cursor is placed on the first letter of the selected row.

Insert the new heading of the ticket with the **UP** and **DOWN** keys.

See paragraph 8.3 Editing.

Pressing the **ENTER key for 3 seconds** the introduced line is confirmed.

Proceed as described for the remaining.

When all lines have been completed press STOP/BACK key to exit.



11.4 Service

Enter password

XX

Insert the code you want with **UP** and **DOWN** keys. Confirm with **ENTER** key.

11.4.1 Setting language

Enter password 03. Confirm with ENTER key.

SELECT LANGUAGE English Enter-Ok Stop-Exit 1

Press the **UP** and **DOWN** keys to select the desired language. Confirm with **ENTER** key.

11.4.2 Date and hour

Enter password 93. Confirm with ENTER key.

Edit Date&time 01/01/17 12:00:00 Enter-OK Stop.Exit

Press the **UP** and **DOWN** keys to select edit the blinking number, press **ENTER** key to edit the next number.

11.4.3 Counters reset

Enter password 05. Confirm with ENTER key.

Refr. recovered q.ty g. Counter reset? Enter-Ok Stop-Exit

Confirm with **ENTER** key. The display shows

Press ENTER key For 3 seconds!

Enter-Ok Stop-Exit

Press ENTER for 3 seconds

Counter reset ok!

Enter-Ok

Confirm with ENTER key.



11.5 A4 Printout

Backup data last job to print In A4? Enter-Ok Stop-Exit

Confirm with ENTER key.

A "Last Job.hst" file is generated and entered on the memory stick, if installed. The file may be imported on a PC and read by means of the "Historical serv & A4 print out.xls" application, which may be downloaded from www.iscsystems.it.

11.6 Back up/restore

Transfer calibrat.
user models and
parameters?
Enter-Ok Stop-Exit

Confirm with **ENTER** key.

Transfer from > to logic board>usb usb>logic board □ Enter-Ok Stop-Exit The name of the file generated is represented by the unit serial no. and it will have the .bck extension (e.g. AP000000.bck).

Press **UP –DOWN** to select desired menu. Press **ENTER** to confirm.

11.7 Exporting service history

Back up of previous services?
Enter-Ok Stop-Exit

Confirm with ENTER key.

The name of the file generated is represented by the unit serial no. and it will have the .hst extension (e.g. AP000000.hst).

A .hst file is generated and entered on the memory stick, if installed. The .hst file may be imported on a PC and read by means of the "Historical serv & A4 print out.xls" application, which may be downloaded from www.iscsystems.it.




11.8 Exporting refrigerant IN/OUT

Back up of previous IN/OUT gas report

Enter-Ok Stop-Exit

Confirm with **ENTER** key.



A .rio file is generated and entered on the memory stick, if installed. The .rio file may be imported on a PC and read by means of the "Refrigerant IN OUT.xls" application, which may be downloaded from www.iscsystems.it.

12 Additional functions

12.1 Leak test with nitrogen (N₂)

The *ICEGARD BLU* is able to test the A/C system with nitrogen (N2). **Not available on HD version.**


The function requires the use of the device charge /discharge N2 (kit 7540004320).



Use only pure nitrogen. Don't use air compressed or other technical gases, see paragraph Errore. L'origine riferimento non è stata trovata. General safety rules

Max test pressure 15 Bar.

Recover and vacuum the A/C systems ,connect the nitrogen supply to the charge/discharge N2 device , and this to the male LP (23) connection in the back of the unit.

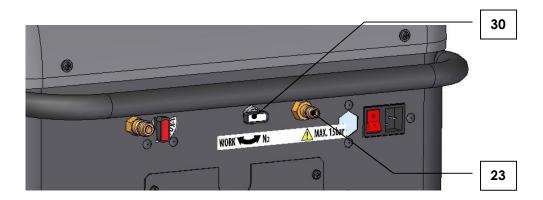




Connect the **LP-HP** (**7-8**) connectors to the A/C system.

Open the connectors by turning the knob clockwise.

The LP-HP gauges indicate the pressure in the two branches of the A/C system.

Turn the nitrogen valve (30) on N2.

Open slowly the charge/discharge N2 valve till the A/C system is charged.

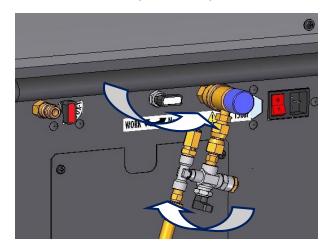

Is possible to check the A/C system with the unit pressure sensor.

When N2 filling is completed, turn valve (30) on WORK, wait few minutes for settlement, then In stand-by mode, press the DOWN Key, the display shows the system pressure in mBar.

When test is complete, is needed to turn the valve (30) in N2 position to discharge the nitrogen.

After discharged, turn again the valve (30) on **WORK** and perform a recovery phase to remove nitrogen residues.

Close the charge /discharge N2 device valve.

Close the valve on the pressure reducer group of the nitrogen tank to stop the nitrogen supply.

Verify possible leakages checking the decay of pressure with the manometer LP (11)during time (5' – 10' depending on the A/C system size).

Using nitrogen with tracer gas (helium) it is possible to search any leak with as sniffer.

At the end of the test, open the charge /discharge N2 device valve to release the nitrogen from the A/C system.

Close the charge/discharge N2 valve.

Turn the nitrogen valve (30) on Work.

Perform 1 minute of vacuum phase.





12.2 Flushing


The **ICEGARD BLU** It is able to perform a flushsing phase to clean a single component or part of the A/C system.

Not available on HD version.

Use the suggested flushing kit 7450007200 to connect the unit at the part of the A/C system to be flushed (see the instruction of the flushing kit).

Connect the charge hose on the connection male HP(24) in the back of the unit. Open the valve (9) to release the refrigerant. Perform a manual recovery phase, see paragraph 9.3 User Program.

To end the flushing phase ,close the valve (9) and wait the automatic stop of the phase.

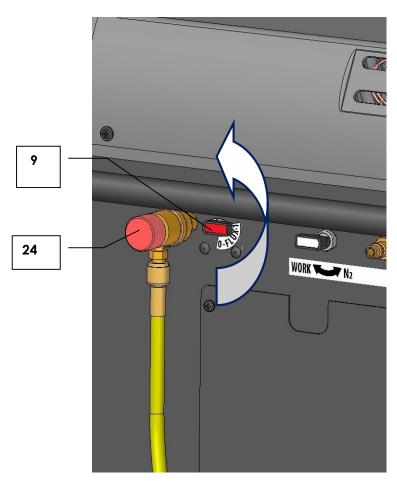

- It is suggest to perform a flushing phase in the follow cases: Replacing of the compressor of the A/C system.
- Moisture or particulate in the A/C system.
- When the cleaning of the A/C systems is in doubt.

To perform a correct flushing phase connect the part to be flashed in manner to allow the flow of refrigerant in the opposite way compared to the normal way of flow. The filling is performed by HP (24), the recovery by LP (7)



12.3 kit POE "Hybrid"

12.3.1 kit POE "Hybrid" enabling

The unit is able to perform a service also on electronic or hybrid cars, with the electrical compressor and not belt driven compressors. These systems contain a type of oil POE with high dielectric resistivity.

Not available on HD version.



The contaminations of these A/C systems with other oil get to decrease its resistivity, creating the risk of electrical shock for the operator.

Work on this A/C systems only if professionally prepared and follow carefully the procedure of this chapter.

For activation of the "Hybrid" function, press the **ENTER** key in stand-by mode:

roi activation of the hybrid function, press the ENTER key in stand-by mode.			
Set plate number Skip data Other menus Enter-Ok Stop-Exit			
Press the UP and DOWN keys to select Other menus . Confirm with ENTER key.			
Int.tank filling Service Print Enter-Ok Stop-Exit			
PAG > POE "Hybrid" ■ POE "Hybrid" > PAG □ Gas Analyzer □ Enter-Ok Stop-Exit			
Press the UP and DOWN keys to select PAG > POE "hybrid" . Confirm with ENTER key.			
Remove squared containers PAG			
Enter-Ok Stop-Exit			
Follow the instructions shown by the display. Confirm with ENTER key.			
Open the LP and HP valve			
Enter-Ok Stop-Exit			
Follow the instructions shown by the display Confirm with ENTED key			

Follow the instructions shown by the display. Confirm with **ENTER** key.




Close nitrogen valve (0)


Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with ENTER key (The valve is placed in the back side of the unit).

Install flushing Device

Enter-Ok Stop-Exit



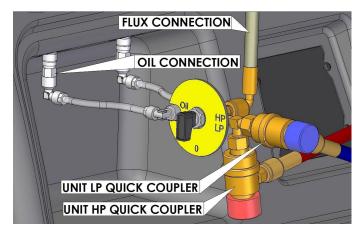


Follow the instructions shown by the display. Confirm with ENTER key.

Turn HP gear Clockwise

Enter-Ok Stop-Exit


Follow the instructions shown by the display.

Confirm with ENTER key. (The valve is placed in the back side of the unit).



Enter-Ok Stop-Exit

Follow the instructions on display. Confirm with ENTER key




N₂ ⚠ MAX. 15bar

Open Flux Valve (1)


Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with **ENTER** key. (The valve is placed in the back side of the unit).



Please wait

The nit performs the I° flushing cycle. At the end buzzer sounds.





Turn device valve On HP/LP position

Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with **ENTER** key.

Turn nitrogen valve on WORK position

Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with ENTER key. (The valve is placed in the back side of the unit).

Please wait

The nit performs the II° flushing cycle. At the and buzzer sounds.

Close Flux Valve(0)

Enter-Ok Stop-Exit

Follow the instructions shown by the display.

Confirm with **ENTER** key. (The valve is placed in the back side of the unit).

The unit completes the recovery of the refrigerant present in the flushing circuit.

Drained oil In progress

Enter-Ok Stop-Exit

Process completed

Enter-Ok Stop-Exit

Confirm with **ENTER** key.

Remove flushing Device

Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with **ENTER** key.

Install rounded containers POE

Enter-Ok Stop-Exit

Follow the instructions shown by the display. Confirm with ENTER key. The display show the stand by mode.







12.3.2 kit POE "Hybrid" disable

In order to disable the "Hybrid" function from the stand by mode press ENTER :
Set plate number Skip data
Other menus ■ Enter-Ok Stop-Exit
Intel or stop lare
Press the UP and DOWN keys to select Other menus . Confirm with ENTER key.
Int.tank filling
Service Print
Enter-Ok Stop-Exit
PAG > POE "Hybrid"
POE "Hybrid" > PAG ■ Gas Analyzer □
Enter-Ok Stop-Exit
Press the UP and DOWN keys to select POE "Hybrid" > PAG. Confirm with ENTER key.
Remove round
Containers POE
Enter-Ok Stop-Exit
Confirm with ENTER key.
Install squared
Containers PAG

Confirm with **ENTER** key. The display show the stand by mode.

Enter-Ok Stop-Exit



.

13 STOP FOR LONG PERIODS

The unit must be stored in a safe place, disconnected from the mains supply and protected from high temperatures, humidity and the risk of collision with other objects that could damage it. Make sure that the valves on the internal tank are closed.

To put the Unit in use, follow the activation procedure **only after having reopened the internal tank** valves.

14 MAINTENANCE

The *ICEGARD BLU* is an extremely reliable unit, built with top-quality components and using the most advanced production technologies.

For these reasons, maintenance is reduced to a minimum, with long intervals between services. Each periodic maintenance operation is monitored by counters. When these counters reach the prescribed count, the following messages are displayed:

Replace filter recycling and vacuum pump oil Enter-Ok

When the maximum quantity of refrigerant for the dehydrator filter is reached, the filter should be replaced and the relative counter returned to zero, ref. subsection 11.4.3 Counters reset

At the same as performing the routine maintenance activities, it is recommended that the pressure sensors be calibrated for the zero points of the scales.

An authorized ISC Systems Customer Service Centre should be contacted for maintenance activities (with the exception of those listed below) and the purchase of spare parts.



14.1 Changing the vacuum pump oil

The vacuum pump oil must be replaced frequently in order to ensure best performances of the unit.

The message mentioned at point **A** will be displayed when the vacuum pump oil needs to be replaced.

To replace the oil, follow these instructions:




DO NOT work on parts of the unit that are not specifically mentioned in this section.

Equipment required:

n°. 1 Screwdriver cross

n°. 2 Hexagonal spanner (10 mm)

- 1. Disconnect the unit from the power supply.
- 2. Remove the 4 screws that secure the lower panel to the unit and remove the panel.
- 3. Place a beaker under the cap (63), open the cap and allow all the oil in the vacuum pump to drain out.
- 4. When the pump has been emptied, screw down cap (63) and open the upper cap (61).
- 5. Fill the pump with oil by pouring it into the upper hole (61) until it reaches halfway up the inspection glass (62).
- 6. Once the pump has been filled, close the upper cap (61).
- 7. Reset the counter. See paragraph 11.4.3 Counters reset.

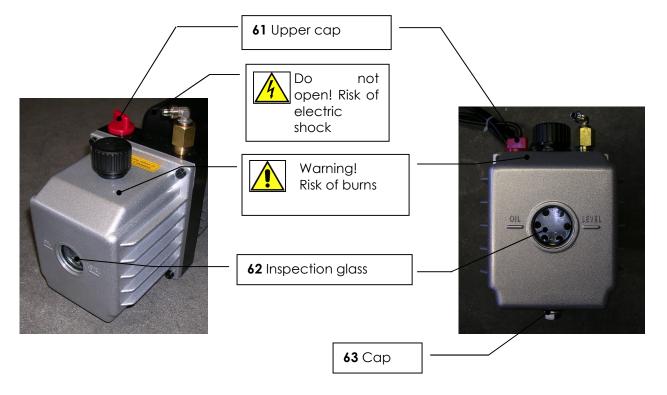



14.2 Filter replacement

The dehydrator filter must be replaced when it is no longer able to absorb the humidity present in the recycled refrigerant.

When the filter needs changing, the message indicated under point **B** appears on the display. To change the filter, follow these instructions:




DO NOT work on parts of the unit that are not specifically mentioned in this section.

Tools required:

n°1 Cross-head screwdriver

n°2 Hexagonal spanner (19 mm + 17 mm)

- 1. Remove the 4 screws that secure the lower panel to the unit and remove the panel.
- 2. Performe a recovery phase, at the end of this phase close immediately the valve (48) to prevent the gas leakages.
- 3. Disconnect the unit from the power supply.
- 4. Using the hexagonal spanners, undo the 2 nuts connected to the filter (15).
- 5. Cut the support band.
- 6. Install the new filter, paying attention to the position of the O-rings and to the arrow direction.
- 7. Using the hexagonal spanners, tighten the 2 nuts connected to the filter (15).
- 8. Install a new band.
- 9. Open the valve (**48**)
- 10. Reset the counter. See paragraph 11.4.3 Counters reset.

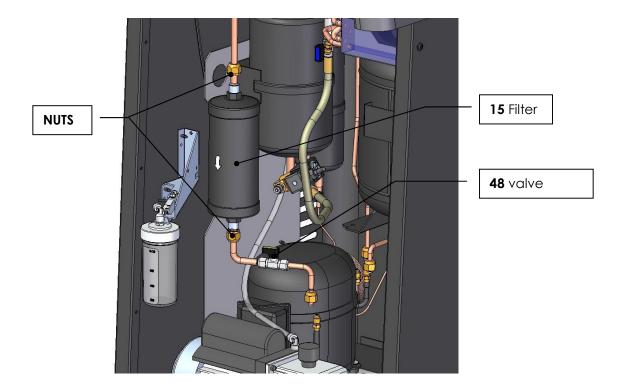



15 DISPOSAL

15.1 Environmental disposals

This product may contain substances that may be dangerous for the environment and cause diseases for Operators if this equipment has not been disposed in the appropriate way.



We inform You about all necessary Information in order to avoid the release of these such dangerous substances and to optimize the use of natural resources. The electrical and electronic equipment must not be disposed with normal urban litters but must be sent to specialized harvest for their appropriate treatment. The symbol of the barred dustbin, that is located on the equipment and on this page, reminds you to pay attention on dispose the product at the end of its lifetime.



In this way, it is possible to avoid that an uncorrect treatment of the substances contained in these such products or an improper use of their parts may cause injurious consequences both for environment and human health.

Furthermore You can give your contribution for recovery, recycling and reutilisation of many row materials contained in these equipments.

For this purpose, both manufacturers and distributors of electric and electronic equipments, organize appropriate harvest centers for the recycling of the same equipments.

At the end of this product lifetime, please contact Your Distributor to have informations about the modalities of harvest.

At the moment of buying a Unit, Your distributor will inform You about the opportunity of giving back - free of charge- another equipment: the necessary requirement is that this equipment has the same typology of use (in this case a Unit for the maintenance of the A/C equipment) and that it can perform the same operative functions of the product previously purchased.

A different disposal of the product from the instruction included in this document will be subjected to the sanctions foreseen by the national laws of the Country where the product will be disposed. We recommend You to adopt further measures favourable to the environment: recycling the internal and external package of the equipment.

Thanks to Your active cooperation, we can reduce concretely the quantity of natural resources employed for the manufacturing of electric and electronic equipments, minimizing the use of discharges for the disposal of the products and improve the standards of life avoiding that dangerous substances would be released in the environment.

15.2 Disposal of recycled material

The refrigerants recovered from systems which cannot be reused must be delivered to the gas suppliers for proper disposal.

The lubricants extracted from systems must be delivered to used oil collection centres.



16 FLOW DIAGRAM

